

# Biolab Medical Unit

9 Weymouth Street, London W1W 6DB, England

Telephone: (+44) 020 7636-5959/5905 Fax: (+44) 020 7580-3910 E-mail: info@biolab.co.uk Internet: www.biolab.co.uk

## Hydrogen Breath Test using Lactose

Reference: **ABCD/XXXX/C19**

Date of birth **07. Jun. 78**

Patient: **Sample Patient**

Sex: **Female**


Referred by: **Dr.....**

Sample date:

Protocol: 25gm of lactose diluted in 200ml of water.

Method: Hydrogen and methane values measured every 60 minutes for 180 minutes.

Basal levels: Hydrogen = 0 ppm Methane = 1 ppm

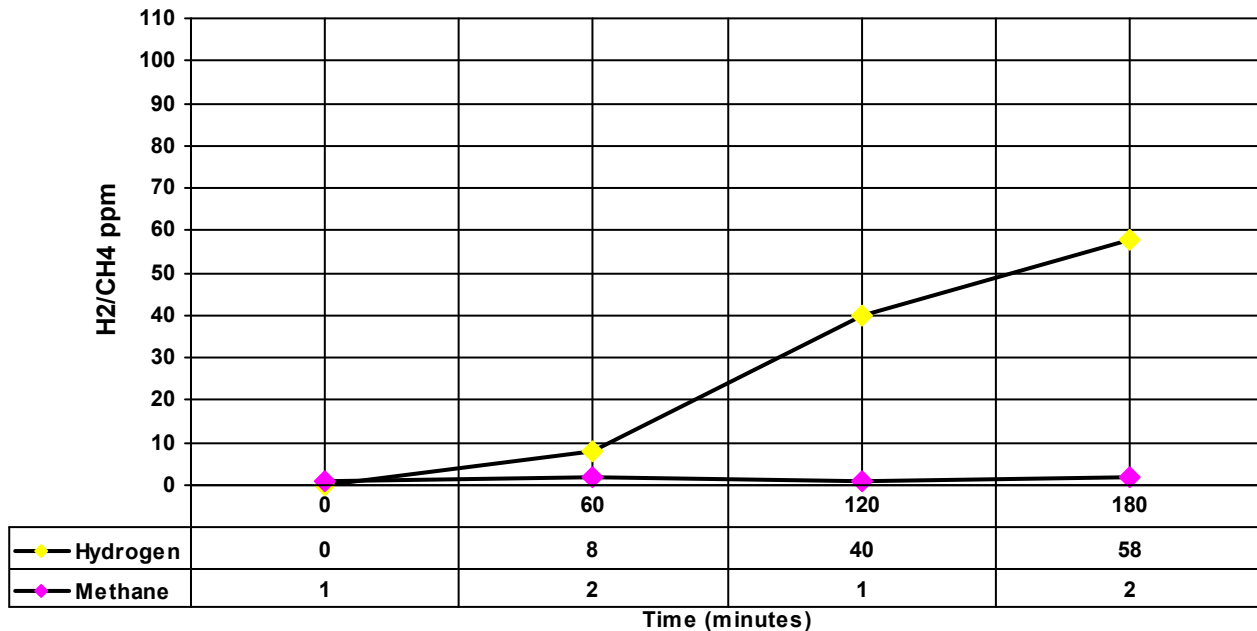

### Comments:

These results indicate lactose intolerance.

### References:

1. Drossman, DA. The functional gastrointestinal disorders and Rome III process. In: Drossman DA, Corazziari E, Delvaux M, Spiller R, Talley NJ, Thompson WG, et. al., eds. Rome III: The Functional Gastrointestinal Disorders. 3rd ed. McLean VA: Degnon Associates; 2006: 1-30.
2. Drossman DA. The functional gastrointestinal disorders and the Rome III process. Gastroenterology. 2006; 130: 1377-90.